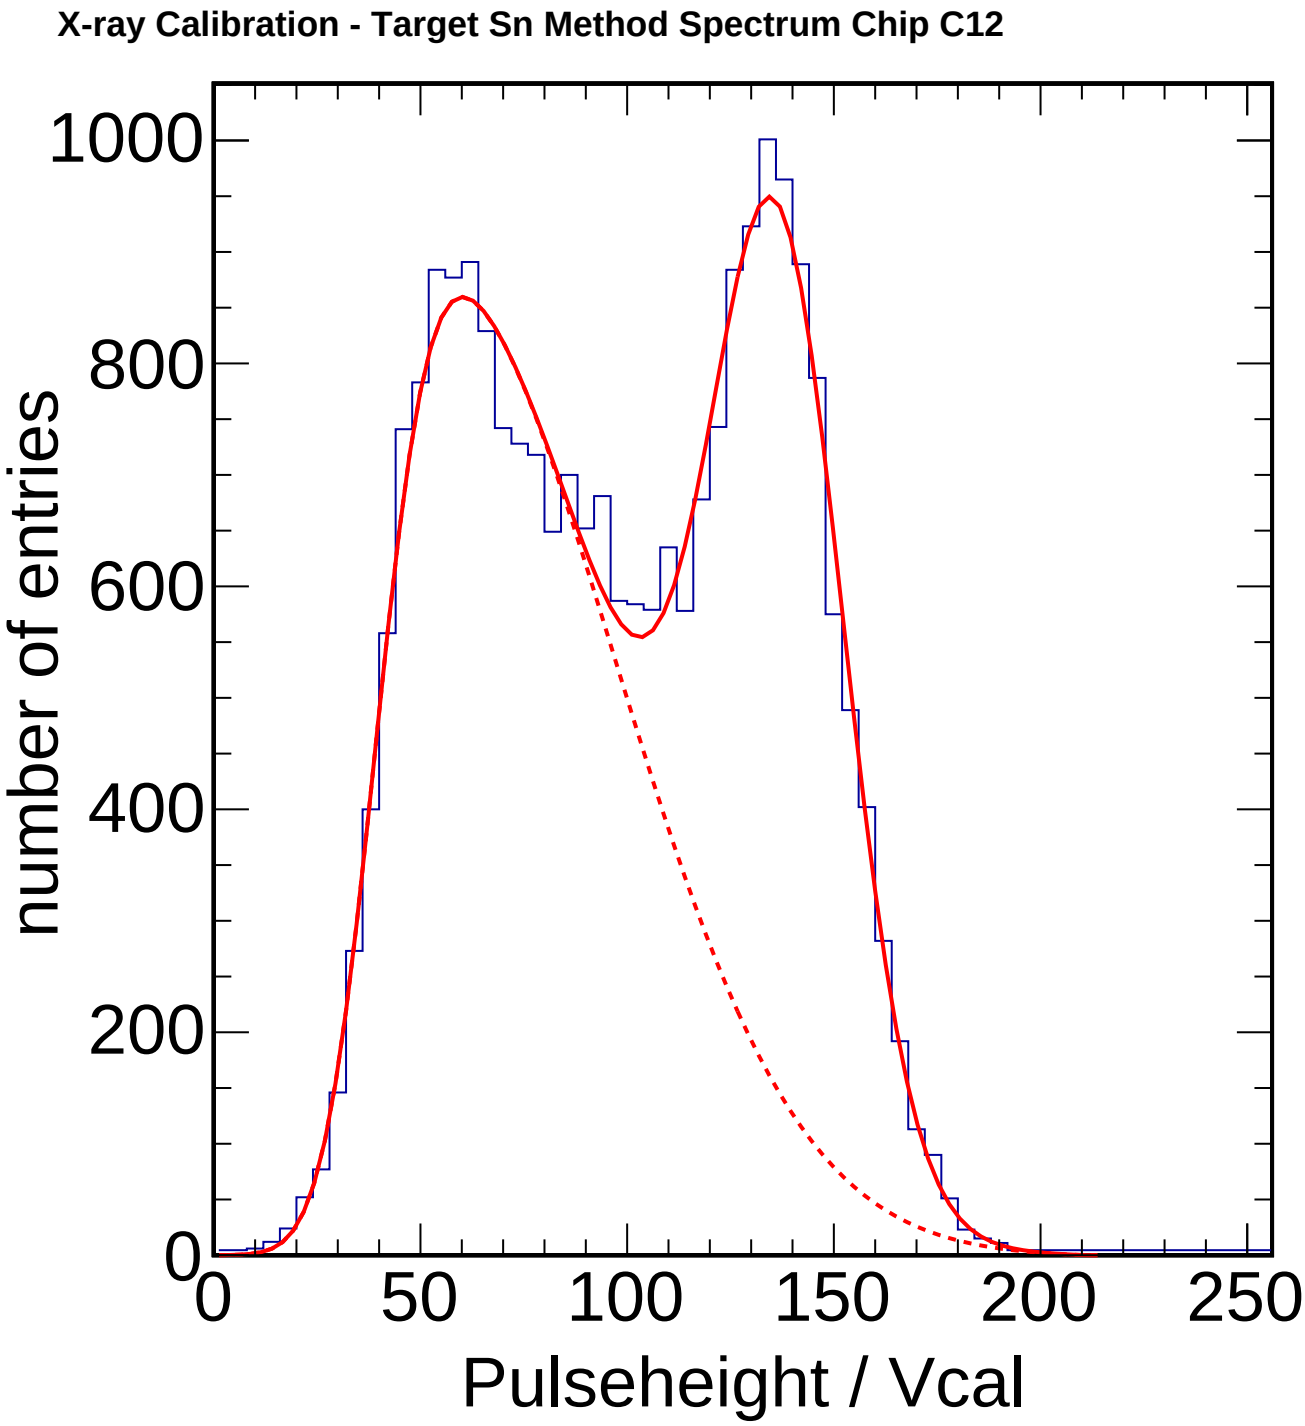
X-ray Calibration - Target Sn Method Spectrum Chip C12
number of entries
Pulseheight / Vcal
0
200
400
600
800
1000
0
50
100
150
200
250